

T2 Estimation Using A Half Fourier Radial Fast Spin-Echo Method

A. Bilgin^{1,2}, Z. Li¹, M. I. Altbach²

¹Dept. of Electrical and Computer Eng., University of Arizona, Tucson, AZ, United States, ²Department of Radiology, University of Arizona, Tucson, AZ, United States

Introduction: Evaluation of the T2 relaxation time holds great potential for diagnosis of pathological disorders. However, the generation of T2 maps is not practical in the clinical setting due to long acquisition times (~ 10 min or longer). Recently, it was demonstrated that high-resolution images at different effective TE (TE_{eff}) values can be generated from a single radial fast-spin echo (RAD-FSE) k-space data set using a simple algorithm^{1,2}. In this method (referred to as the “multi-tier” method), images at various TE_{eff} are generated by including data acquired at a specific TE in the central part of k-space up to a radius determined by the Nyquist criteria. Beyond this first Nyquist radius, views acquired at other TE values are included gradually as illustrated in Fig. 1. The images at different TE_{eff} values are then used to estimate high-resolution T2 maps. With this methodology T2 maps can be obtained rapidly (e.g. a breath hold).

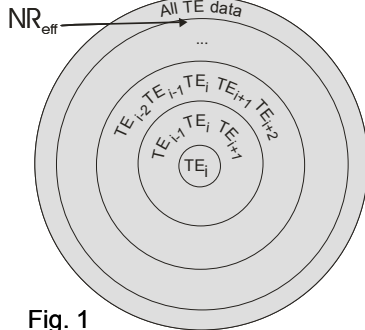


Fig. 1

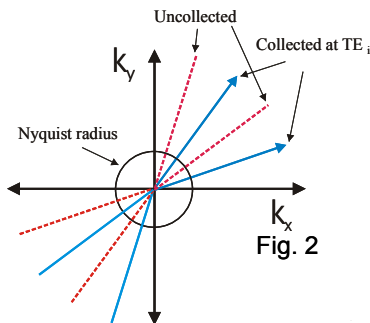


Fig. 2

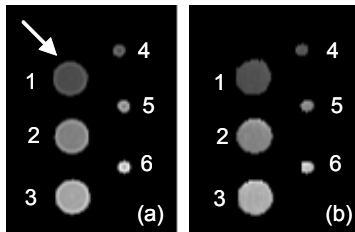


Fig. 3. T2 maps reconstructed from: (a) 256 full views, (b) 256 bent views.

Table 1: Comparison of T2 values obtained from different methods. %Δ indicates the % difference with respect to the gold standard.

Object	Gold Std.	256 Full Views		256 Bent Views	
	Mean T2	Mean T2	% Δ	Mean T2	% Δ
1	104.02	110.25	6	105.93	2
2	174.07	185.34	6	178.04	2
3	247.81	231.56	7	232.39	6
4	106.92	130.33	22	115.92	8
5	178.75	209.08	17	183.75	3
6	245.22	269.00	10	256.56	5

in Table 1. The T2 maps are shown in Fig. 3. The results indicate that the T2 bias for small objects is significantly reduced with bent-RAD-FSE. Also, note that the edge artifacts in the full-view T2 maps illustrated by the arrow in Fig. 3 are significantly reduced in the bent T2 maps.

Conclusion: A method based on a bent k-space trajectory and half Fourier reconstruction was developed for obtaining high-resolution T2 maps from a single RAD-FSE k-space data set. With this method the effective Nyquist radius (NR_{eff}) is doubled compared to the conventional radial k-space trajectory where a full k-space line is acquired per readout period without increasing imaging time. This significantly reduces the T2 bias for small objects. The proposed method may lead to accurate diagnosis of pathologies in small lesions. Further improvements can be achieved using parallel imaging techniques or iterative T2 estimation methods.

Acknowledgements: Work supported by NIH (CA099074) and the American Heart Association (0355490Z).

References: [1] Song HK, MRM, 44, 825 (2000). [2] Altbach MI, JMRI, 16, 179 (2002). [3] Altbach MI, MRM, 54, 549 (2005). [4] Noll DC, IEEE TMI, 10, 154 (1991). [5] Noll DC, Proc. SPIE, 1443, 29 (1991). [6] Block WF, Proc. ISMRM, (1999). [7] Toropov, Proc. ISMRM (2001). [8] Bilgin A, Proc. ISMRM, (2004). [9] Bilgin A, Proc. ISMRM, (2005).