

Comparison of Linear and Non-linear Fitting Methods for Estimating T1 from SPGR Signals

L-C. Chang¹, C. Koay¹, S. Deoni², and C. Pierpaoli¹

¹NICHD, NIH, Bethesda, MD, United States, ²Centre for Neuroimaging Sciences, Institutes of Psychiatry, King's College London, London, United Kingdom

Introduction: T_1 maps can be computed from spoiled gradient recalled echo (SPGR) images acquired with different repetition times (TR s) and/or flip angles. Recently, the acquisition of high resolution T_1 maps in a clinically feasible timeframe has been demonstrated with Driven Equilibrium Single Pulse Observation of T_1 (DESPO1) [1]. DESPO1 derives T_1 from two or more SPGR images acquired with constant TR and different flip angles using linear least-squares (LS) fitting of a linear transformation of the function relating signal intensity, flip angle, TR , T_1 and equilibrium longitudinal magnetization [1, 2]. Linear fitting has the advantage of being computationally fast, however, non-linear fitting approaches could be preferable if they provide better accuracy and precision of the estimated T_1 . Few papers have investigated the impact of fitting procedures on the precision of T_1 estimated from SPGR signals [1-3], but the impact on T_1 accuracy is essentially unexplored. Here, we provide a systematic evaluation of accuracy and precision of T_1 calculated with both linear and non-linear fitting methods using Monte Carlo simulations of sets of SPGR signals produced assuming various experimental conditions.

Method: The measured SPGR signal intensity can be written as $S_i = \frac{M_0(1 - E_1)\sin(\alpha)}{1 - E_1\cos(\alpha)} + N_i$ (1), where α is the flip angle, M_0 is the equilibrium

longitudinal magnetization, N_i is the random noise function, and $E_1 = \exp(-\frac{TR}{T_1})$ [1, 2]. The non-linear LS approach estimates T_1 and M_0 from

equation (1) by minimizing the equation: $f_{NLS}(\hat{M}_0, \hat{T}_1) = \sum_{i=1}^n (S_i - \hat{S}_i)^2$. We tested two non-linear fitting methods, Levenberg-Marquardt (LM) [4] and Modified Full Newton (MFN) [5]. Linear fitting can be used if all images in the dataset are collected with the same TR and the noise term is

neglected. Under these conditions equation (1) can be represented in linear form as: $\frac{S_i}{\sin(\alpha)} = E_1 \frac{S_i}{\tan(\alpha)} + M_0(1 - E_1)$ (2). We used a linear LS method

to compute T_1 and M_0 from equation (2) similarly to what was previously proposed [1, 2].

Simulations: We performed simulations of different experimental designs, (TR s, flip angles) and different expected values of T_1 . Different signal to noise (SNR) levels were simulated by adding (in quadrature) Gaussian noise with zero mean and variable standard deviation (σ) to the noise-free SPGR signals generated using equation (1). Results reported below are computed assuming $TR=10$ ms, $T_1=1000$ ms and $M_0=3000$, optimal flip angles [2] of 19.3 and 3.4 degrees, 2, 4, 6, 8, 16, or 32 SPGR images with repeated optimal angles, and SNR (expressed as M_0/σ) ranging from 100 to 600.

Results: Figure 1 shows the distributions of T_1 obtained with linear and nonlinear methods at two different SNR levels. The variability of T_1 is similar in both linear and nonlinear cases but the distribution of T_1 is biased (shifted to the left) in the linear case. This bias is more pronounced at low SNR. Figures 2 and 3 show the mean and the standard deviation (SD) of T_1 as a function of the number of data points. As the number of data points increases, the SD decreases for both the linear and non-linear cases. Surprisingly the mean value appears progressively more biased as the number of data points increases when linear fitting is used (Fig. 2). At very low SNR, the estimated T_1 using LM non-linear fitting was found to be unstable with a high occurrence of negative T_1 values; the MFN approach was less susceptible to this problem (data not shown).

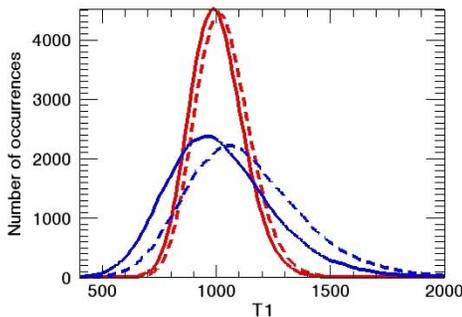


Fig. 1 The distribution of T_1 using 6 points (3 replicates of optimal angles) with 2 different noise levels. (red: $M_0/\sigma=200$, blue: $M_0/\sigma=100$, solid line: non-linear, dashed line: linear) The true T_1 value is 1000 ms.

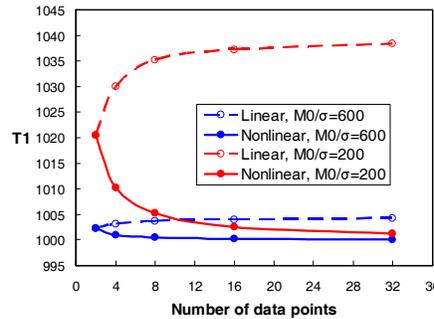


Fig. 2 Mean estimated T_1 value using linear and non-linear methods with increasing number of data points and at different noise levels (red: $M_0/\sigma=200$ and blue: $M_0/\sigma=600$). The true T_1 value is 1000 ms.

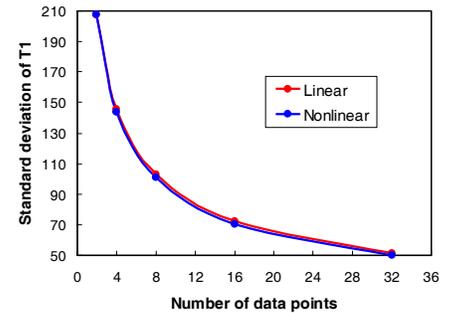


Fig. 3 The standard deviation of T_1 using linear and non-linear fitting with increasing number of data points ($TR=10$ ms, $T_1=1000$ ms $M_0/\sigma=200$).

Discussion: The main goal of this study was to establish if fitting SPGR data to a non-linear model would provide better estimates of T_1 than the conventional approach of fitting data to a linear model. Regarding T_1 variance, linear and non-linear approaches appear equivalent over a wide range of experimental conditions. However, T_1 estimates using linear fitting are biased. The accuracy of T_1 is improved as the number of data points is increased with non-linear fitting, but paradoxically is decreased with linear fitting. Overall, non-linear fitting would appear to be the preferred method for computing T_1 from SPGR data, however, the instability of non-linear fitting at low SNR is disconcerting. We suspect that this instability is due to the known large residuals problem [4], but more work is needed to fully elucidate T_1 estimation in the low SNR regime.

Reference: [1] Deoni et al, *Magn Reson Med* 49: 515-526, 2003. [2] Wang et al, *Magn Reson Med* 5: 399-416, 1987. [3] Deoni et al, *Magn Reson Med* 51: 194-199, 2004. [4] Nocedal et al, *Numerical Optimization*, Springer, 1999. [5] Koay et al, *J. Magn Reson.* 182:115-125, 2006