

## In vivo detection of hyperpolarized $^{15}\text{N}$ Choline in the rat

C. Cudalbu<sup>1</sup>, A. Comment<sup>2</sup>, K. Uffmann<sup>1</sup>, R. B. van Heeswijk<sup>1</sup>, C. Perazzolo<sup>1</sup>, F. Kurdzesau<sup>2,3</sup>, S. Jannin<sup>2</sup>, V. Denisov<sup>4</sup>, D. Kirik<sup>4</sup>, J. J. vna der Klink<sup>2</sup>, and R. Gruetter<sup>1,5</sup>

<sup>1</sup>Laboratory for Functional and Metabolic Imaging, Ecole Polytechnique Federale de Lausanne, Lausanne, Switzerland, <sup>2</sup>Laboratory for Physics of Nanostructured Materials, Ecole Polytechnique Fédérale de Lausanne, Lausanne, Switzerland, <sup>3</sup>Paul Scherrer Institute, Villigen, Switzerland, <sup>4</sup>Department of Experimental Medical Science Brain Repair and Imaging in Neural Systems (BRAINS), Lund University, Sweden, <sup>5</sup>Departments of Radiology, Universities of Lausanne and Geneva, Switzerland

### Introduction:

$^{15}\text{N}$  MRS labeled experiments are especially useful for measuring the rates of synthesis and turnover of amino acids such as glutamate and glutamine, implicated in glutamate neurotransmission (1). However, the very low natural abundance of  $^{15}\text{N}$  (0.365%) makes the study of nitrogen metabolism difficult. A recent study has reported relatively long  $T_1$  for some nitrogen compounds (i.e. Choline) (2), suggesting that  $^{15}\text{N}$  may be a suitable candidate to be used with hyperpolarization by means of DNP (3). This is of special interest for observing phospholipid metabolism in cancer due to changes in choline metabolism (2). The aim of the present study was to demonstrate the feasibility of detecting hyperpolarized  $^{15}\text{N}$  labeled Choline *in vivo* in the rat.

### Methods:



All the  $^{15}\text{N}$  MRS data were acquired on a 9.4T system (Varian/Magnex Scientific) using a home-built quadrature  $^1\text{H}$  coil with a single 5-loop 10 mm  $^{15}\text{N}$  coil placed on the head of the animal. For the *in vivo* experiments, male Sprague-Dawley rats (~350g) were anesthetized using 1.5% isoflurane and a femoral vein was catheterized for injection. Blood pressure, respiration rate and temperature were maintained within normal range.

$^{15}\text{N}$  choline chloride (Sigma Aldrich) solution, prepared at a concentration of 6M in a deuterated water-glycerol solvent doped with 50mM of TEMPO as free radical, was polarized at 3.35 T and 1.2 K using a polarizer described in (4). After dissolution into 5 ml of  $\text{D}_2\text{O}$ , the  $^{15}\text{N}$  Cho chloride sample was automatically transferred to a phase separator placed in the bore of the 9.4T system within 6s. An external pump then injected 2.5 ml of the sample over 8s into the rat femoral vein. The concentration of the  $^{15}\text{N}$  Cho infusate was ~90mM. The injection was repeated two times on the same animal. The *in vitro* and *in vivo* acquisitions were performed using a 3ms  $10^\circ$  BIR4 pulse with 3s interpulse delay. The FIDs were analyzed with AMARES (5).

### Results and Discussions:

The polarization in the cryostat reached 4% (corresponding to ~10000 times amplification compared to room temperature polarization at 9.4T). The maximum polarization was obtained after ~2hours, within 1600 s time constant.

*In vivo*  $^{15}\text{N}$  Cho was discernible above the noise level for about the first ~90 s (Figure 1, 2) and the linewidth was 9 Hz. The fit for the *in vivo*  $^{15}\text{N}$  Cho  $T_1$  estimation was performed on the last part of the time course shown in Figure 1, from 27 to 105 s. Taking into account the RF flip angle correction, the  $T_1$  was estimated to be approximately 150 s *in vitro* and around 1min *in vivo*. The *in vitro* results on phantom were in agreement with the one *in vitro* study using  $^{15}\text{N}$  hyperpolarized Cho (2). The long  $T_1$  combined with the potential to observe hyperpolarized  $^{15}\text{N}$  Cho *in vivo* makes this compound useful for early detection of tumors and also for a potential utilization in the assessment of blood flow. The relatively long  $T_1$  of the nitrogen atom may render other nitrogen compounds suitable for DNP studies such as this one. To our knowledge the *in vivo* detection of hyperpolarized  $^{15}\text{N}$  has not been demonstrated to date. We conclude that it is feasible to detect hyperpolarized  $^{15}\text{N}$  in live animals.

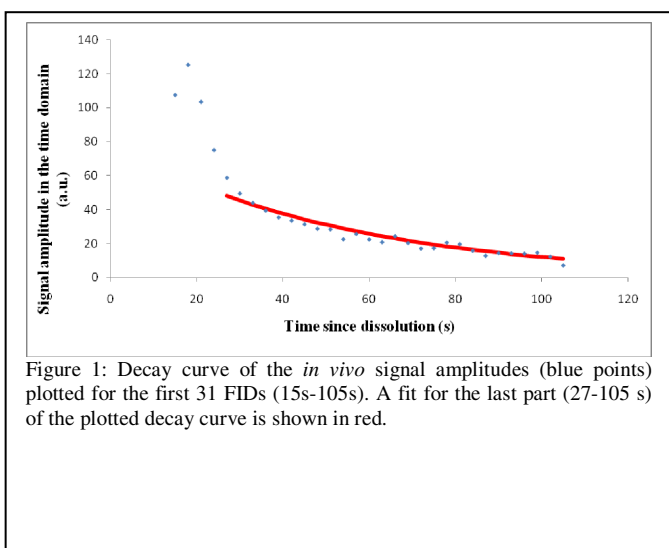

### References:

[1] Farrow et al., *Biochem J* 270 (1990) 473. [2] Eykyn et al., *ISMRM* (2007), 1319. [3] Abragam and Goldman; *Rep Prog Phys* 41 (1978) p395. [4] Comment et al., *Conc Magn Reson* 31B (2007) p255. [5] Vanhamme et. al., *J. Magn. Reson.* 129 (1997) 35.

**Acknowledgements.** Supported by Centre d'Imagerie BioMédicale (CIBM) of the UNIL, UNIGE, HUG, CHUV, EPFL and the Leenaards and Jeantet Foundations; SNF grant 3100A0-116220